



® DenTag

101%
italian
Quality




50 Strumenti da laboratorio · Instruments for laboratory

Instruments pour laboratoire ·

Instrumentos para laboratorio




50
2

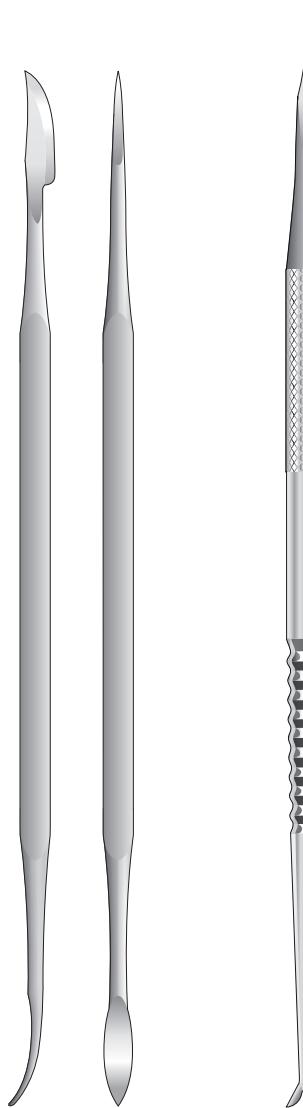


Hylin

5000.B0.00

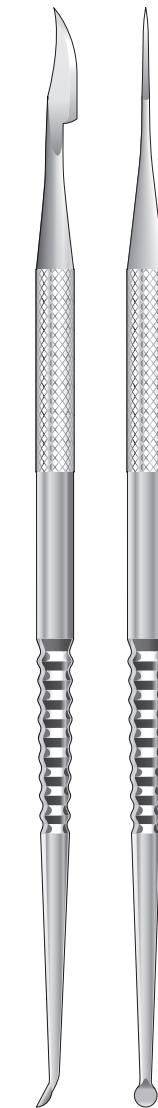

Hylin-Le Cron

5000.B0.01

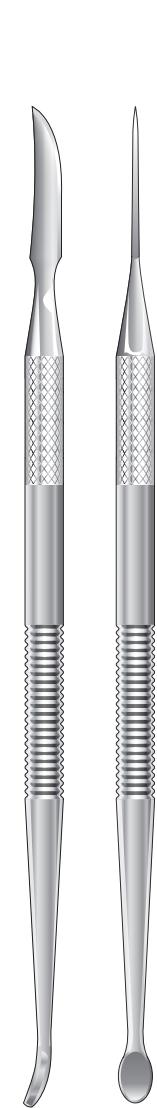

Hylin ceramic

5000.B0.02

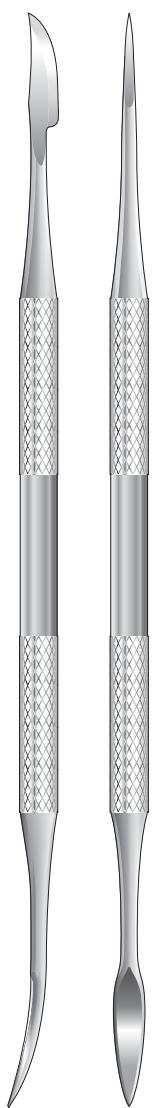


fig. 3

5000.B0.03


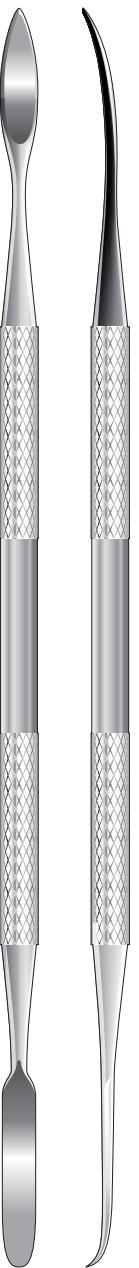


fig. 4

5000.B0.04

Strumenti da laboratorio
Instruments for laboratory
Instruments pour laboratoire
Instrumentos para laboratorio

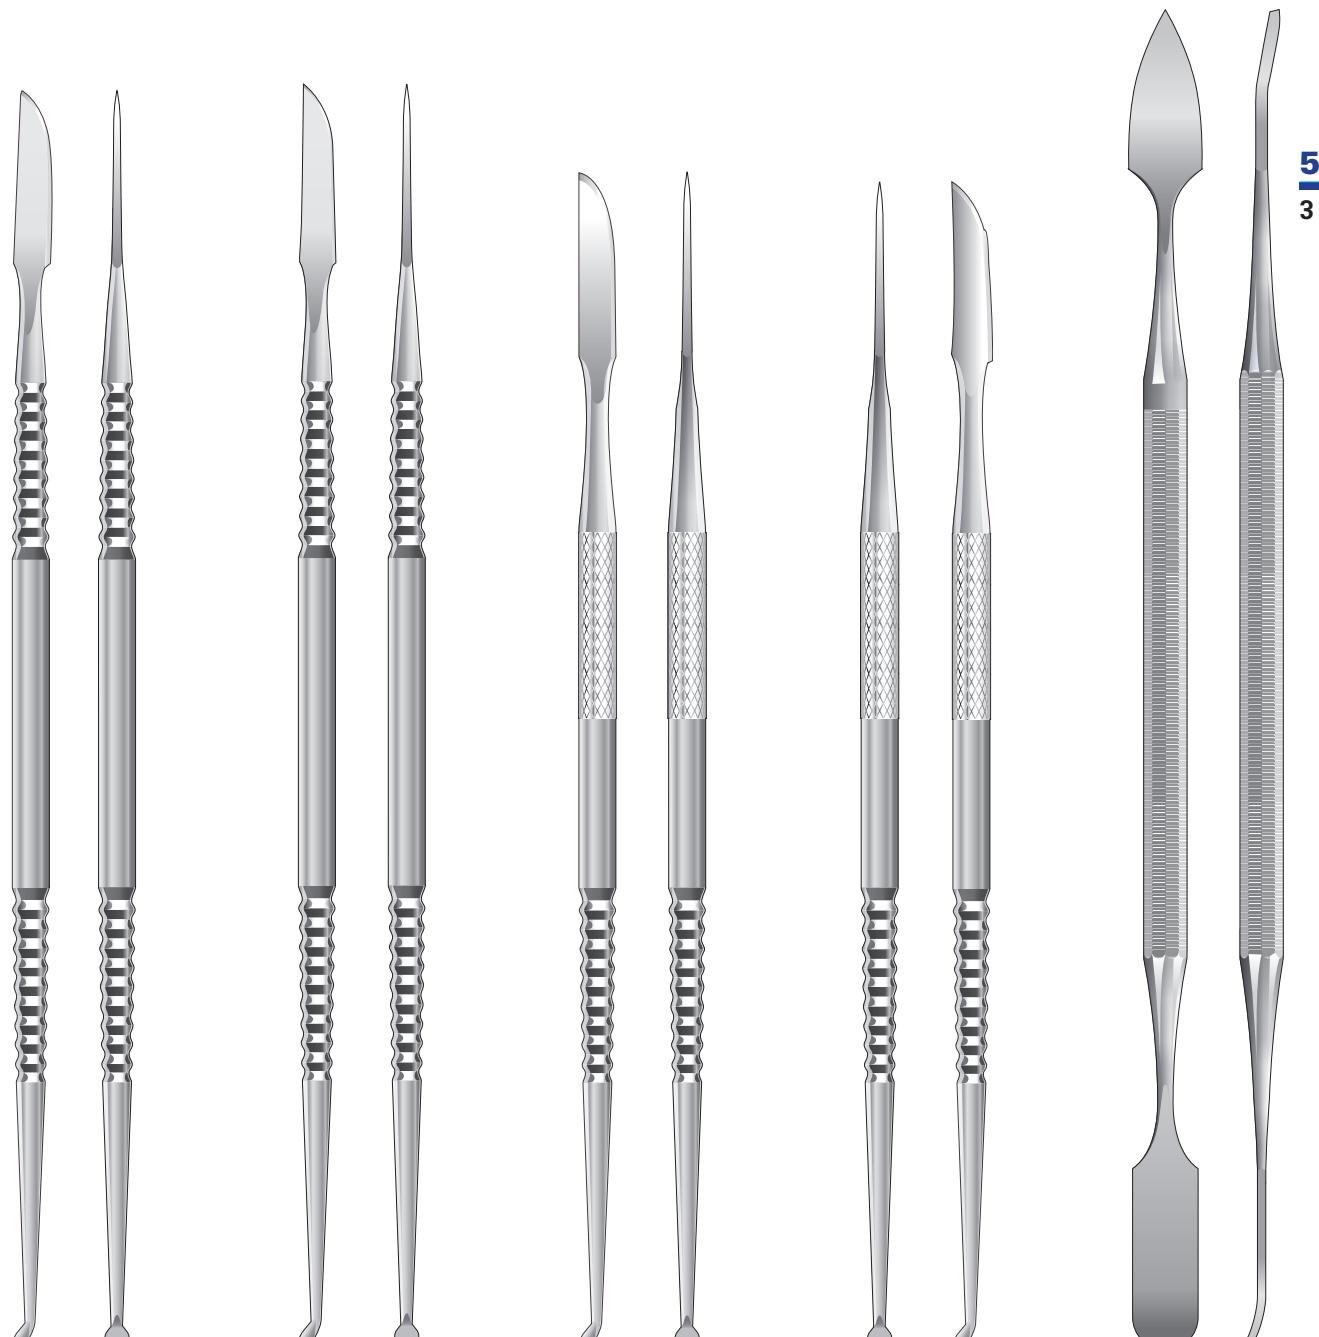

Le Cron fig. 5

5000.B0.05

Le Cron fig. 6

5000.B0.06

Le Cron fig. 7


5000.B0.07

Le Cron fig. 8

5000.B0.08


Gritman fig. 13

5000.E0.13

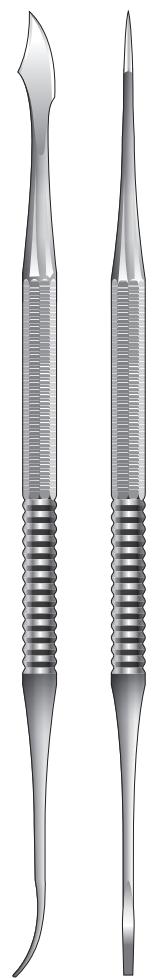


Zahle fig. 9

5000.E0.09

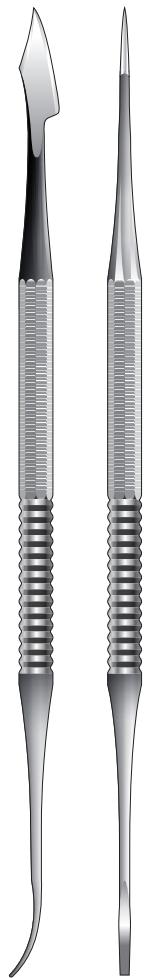


Zahle fig. 10

5000.E0.10

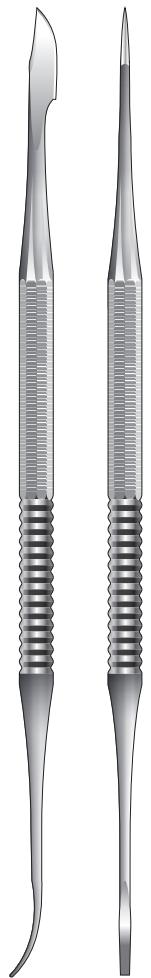


Zahle fig. 11

5000.E0.11

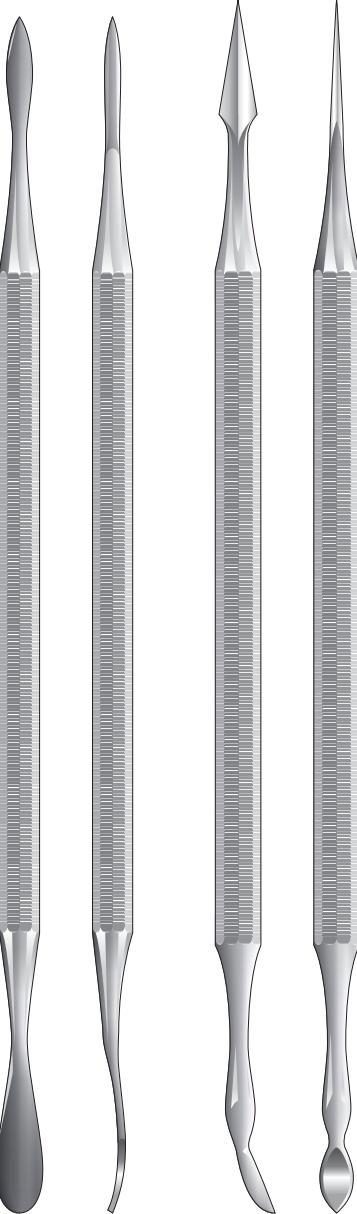


Beale fig. 14

5000.E0.14

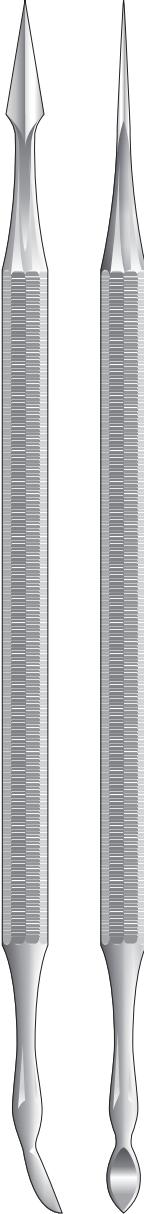

Roach fig. 15

5000.E0.15

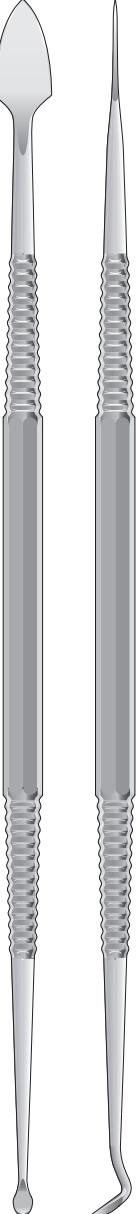

Vehé fig. 16

5000.E0.16

Strumenti da laboratorio
Instruments for laboratory
Instruments pour laboratoire
Instrumentos para laboratorio

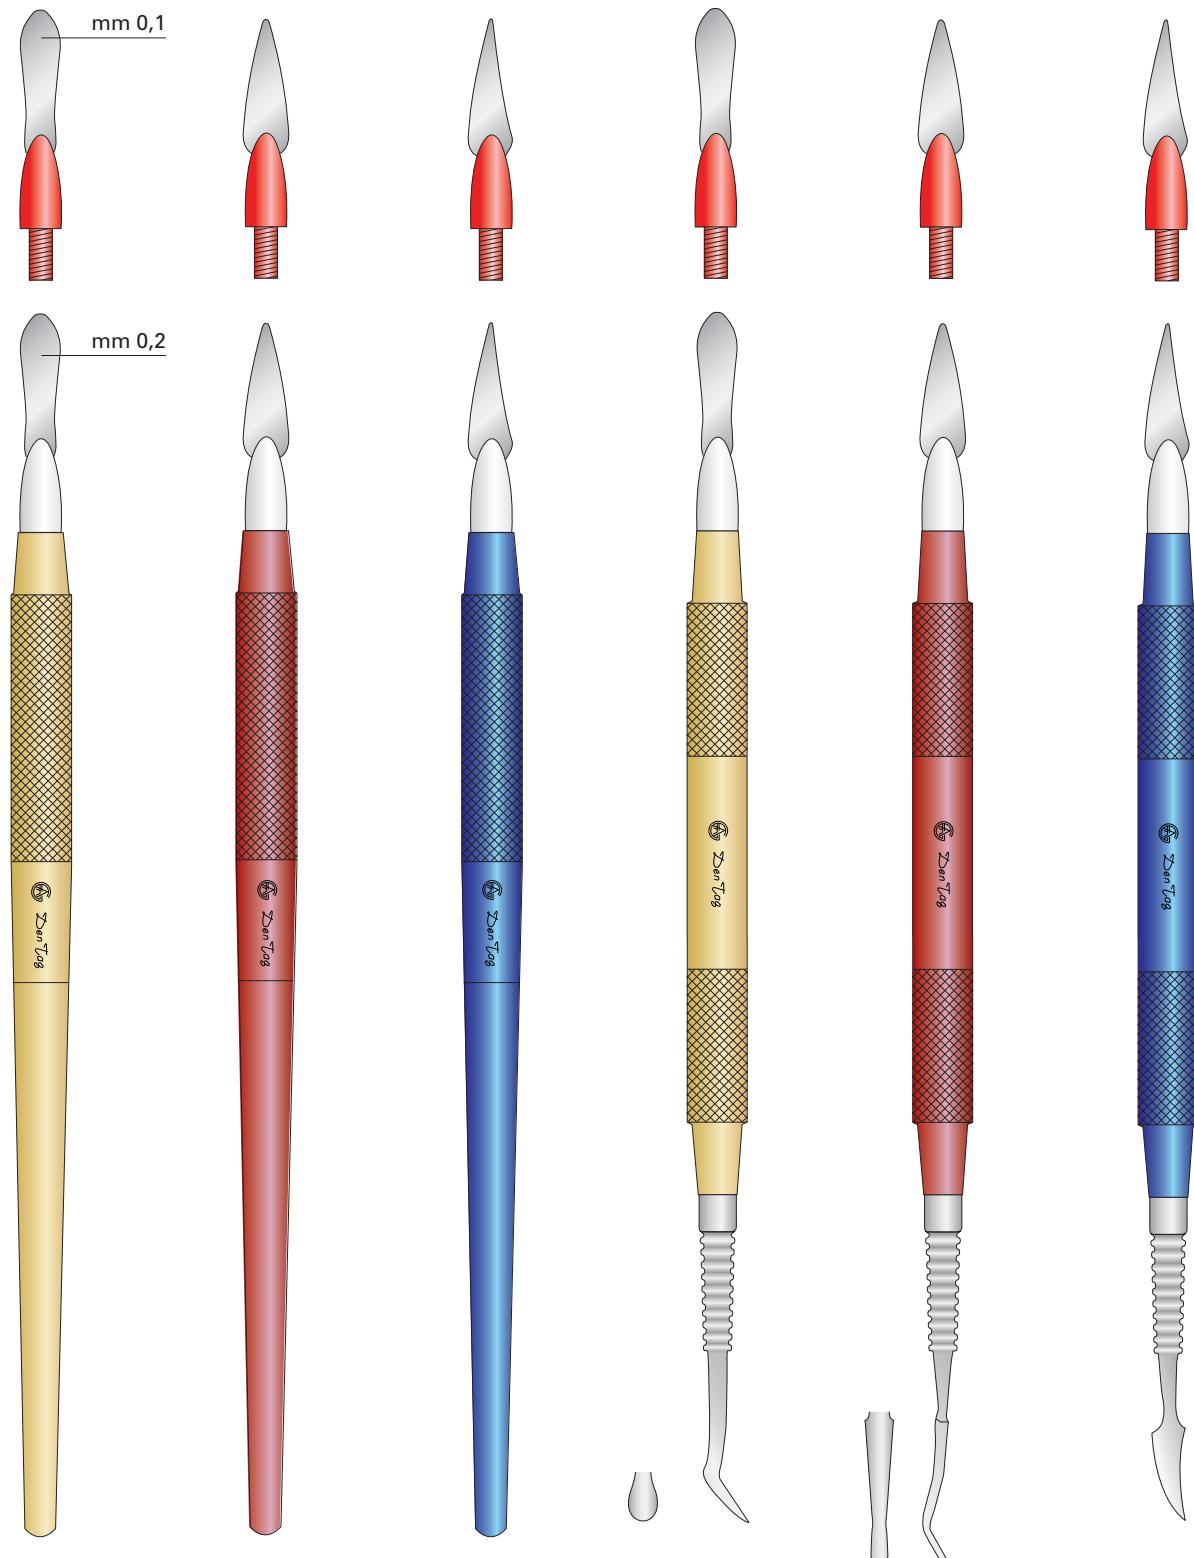


fig. 11

5001.L0.11
 DT06 • DT08
 A0 • G0

fig. 12

5001.L0.12
 DT06 • DT08
 A0 • G0

fig. 13

5001.L0.13
 DT06 • DT08
 A0 • G0

fig. 11

5002.L0.11
 DT06 • DT08
 A0 • G0

fig. 12

5002.L0.12
 DT06 • DT08
 A0 • G0

fig. 13

5002.L0.13
 DT06 • DT08
 A0 • G0

Greenstein




Dentag

Strumenti da laboratorio
Instruments for laboratory
Instruments pour laboratoire
Instrumentos para laboratorio

50

6

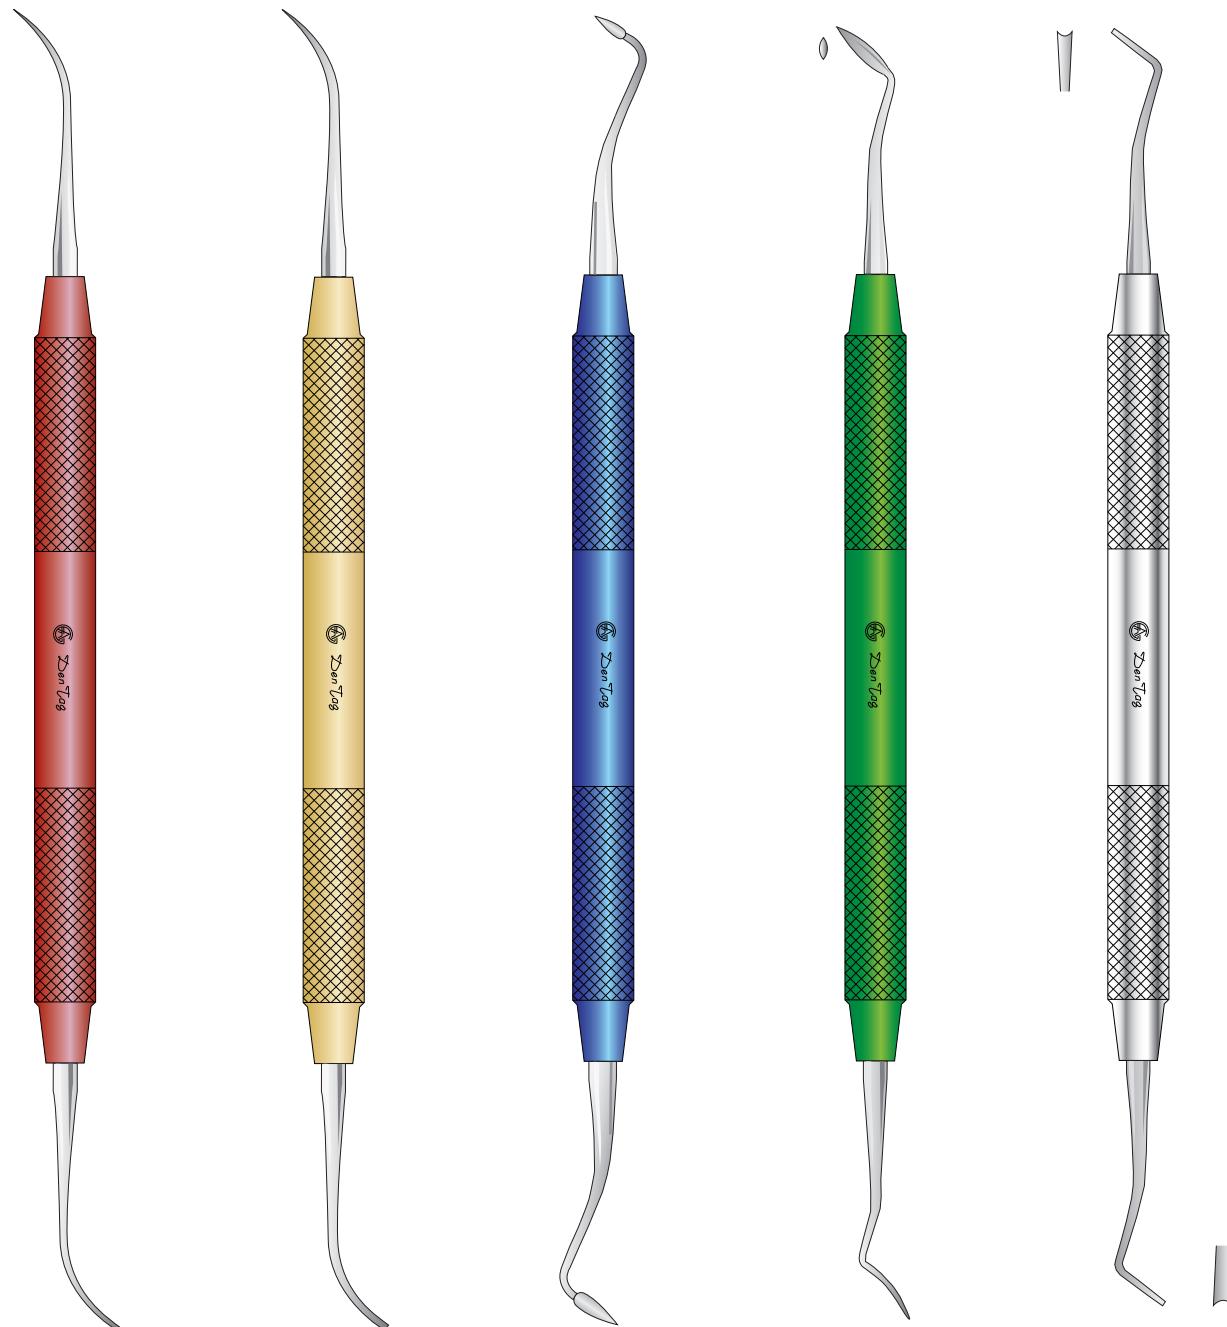

P.K. Thomas fig. 1

5003.L0.01

DT06 • DT08
A0 • G0

P.K. Thomas fig. 2

5003.L0.02

DT06 • DT08
A0 • G0

P.K. Thomas fig. 3

5003.L0.03

DT06 • DT08
A0 • G0

P.K. Thomas fig. 4

5003.L0.04

DT06 • DT08
A0 • G0

P.K. Thomas fig. 5

5003.L0.05

DT06 • DT08
A0 • G0